

WHEELCHAIR BACKREST CONFIGURATION FOR TENSION ADJUSTABLE BACKRESTS


QMF 54

Client Ref:	
Wheelchair Make/Model:	
Wheelchair Size:	
Form Completed By:	Date:
Wheelchair Service:	

NOTE:

Where a Bracing Bar (X) is used, is it possible to secure the Tension Adjustable Backrest at the front of the wheelchair back posts ?

YES NO

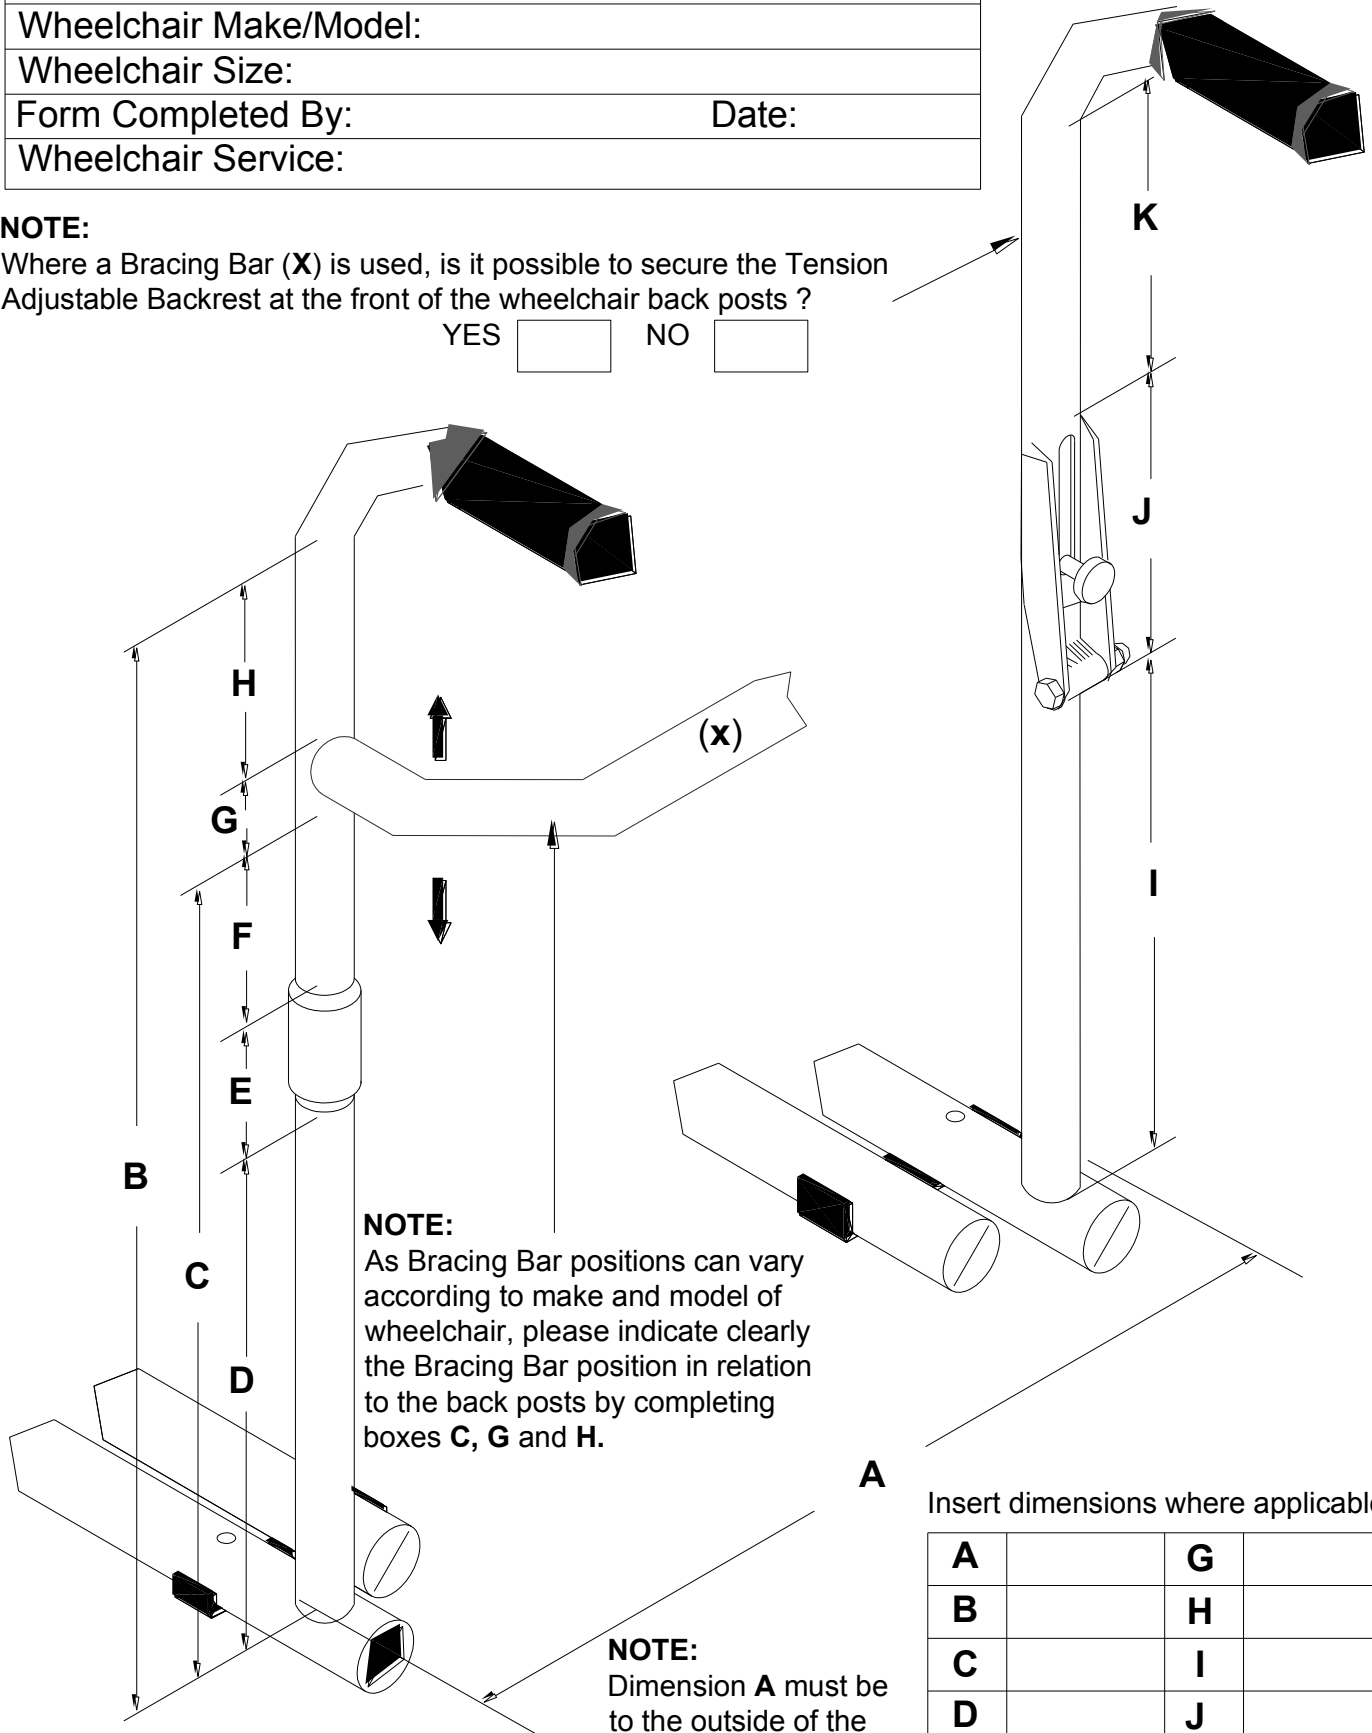

NOTE:
As Bracing Bar positions can vary according to make and model of wheelchair, please indicate clearly the Bracing Bar position in relation to the back posts by completing boxes C, G and H.

NOTE:
Dimension A must be to the outside of the back posts.

Insert dimensions where applicable.

A		G	
B		H	
C		I	
D		J	
E		K	
F			